



# Future

Cytometer:	LSRII	User:	Administrator
Cytometer Name:	LSRII	Institution:	
Serial Number:	1	Software:	BD FACSDiva 6.2
Input Device:	Manual	Date:	10/6/2011 2:07:08 PM
Window Extension:	10.00		


Blue Laser  
(488nm)  
FSC

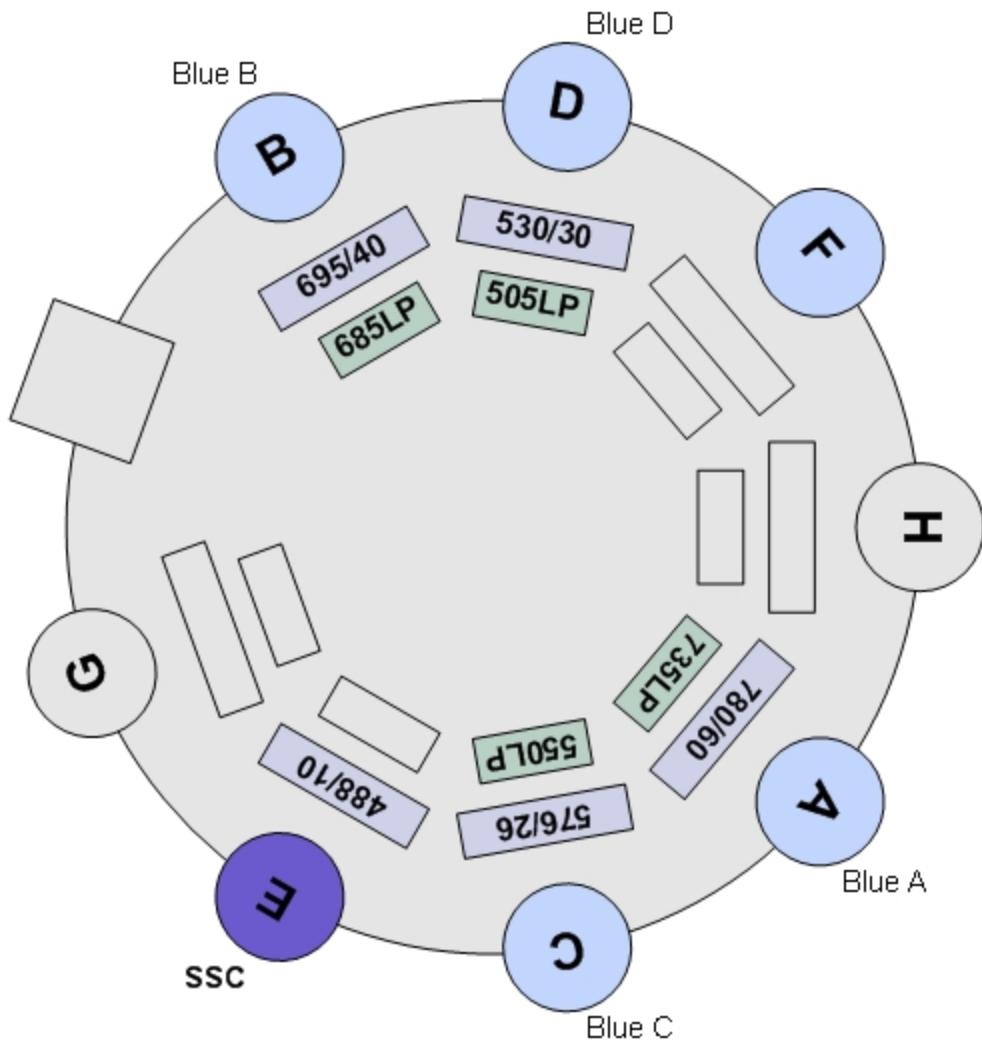


Yellow Green Laser  
FSC

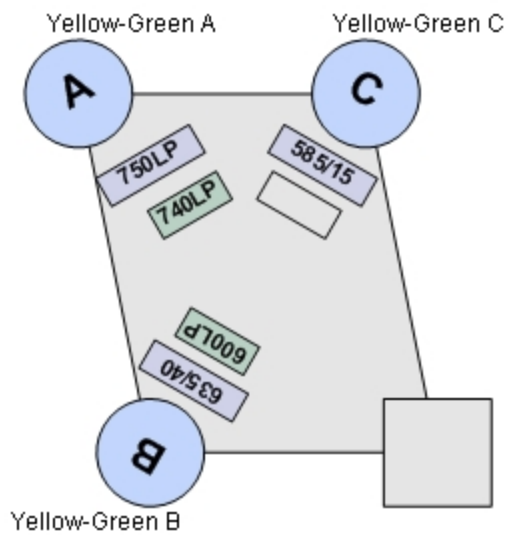

355 UV Laser  
(355nm)

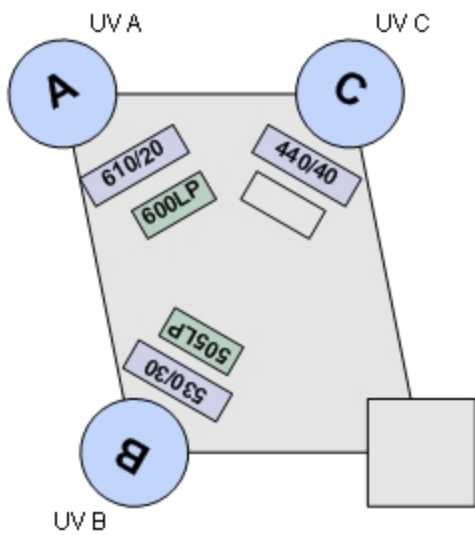

Red Laser  
(633nm)

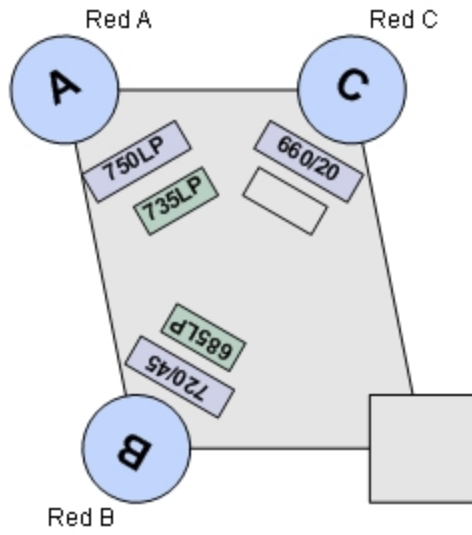

Comments: