



## 6 Blue, 3 YellowGreen, 3 Red, 3 UV

Cytometer:	LSRII	User:	Administrator
Cytometer Name:	LSRII	Institution:	
Serial Number:	1	Software:	BD FACSDiva 6.2
Input Device:	Manual	Date:	6/16/2015 8:04:16 AM
Window Extension:	10.00		


Blue Laser  
(488nm)  
FSC

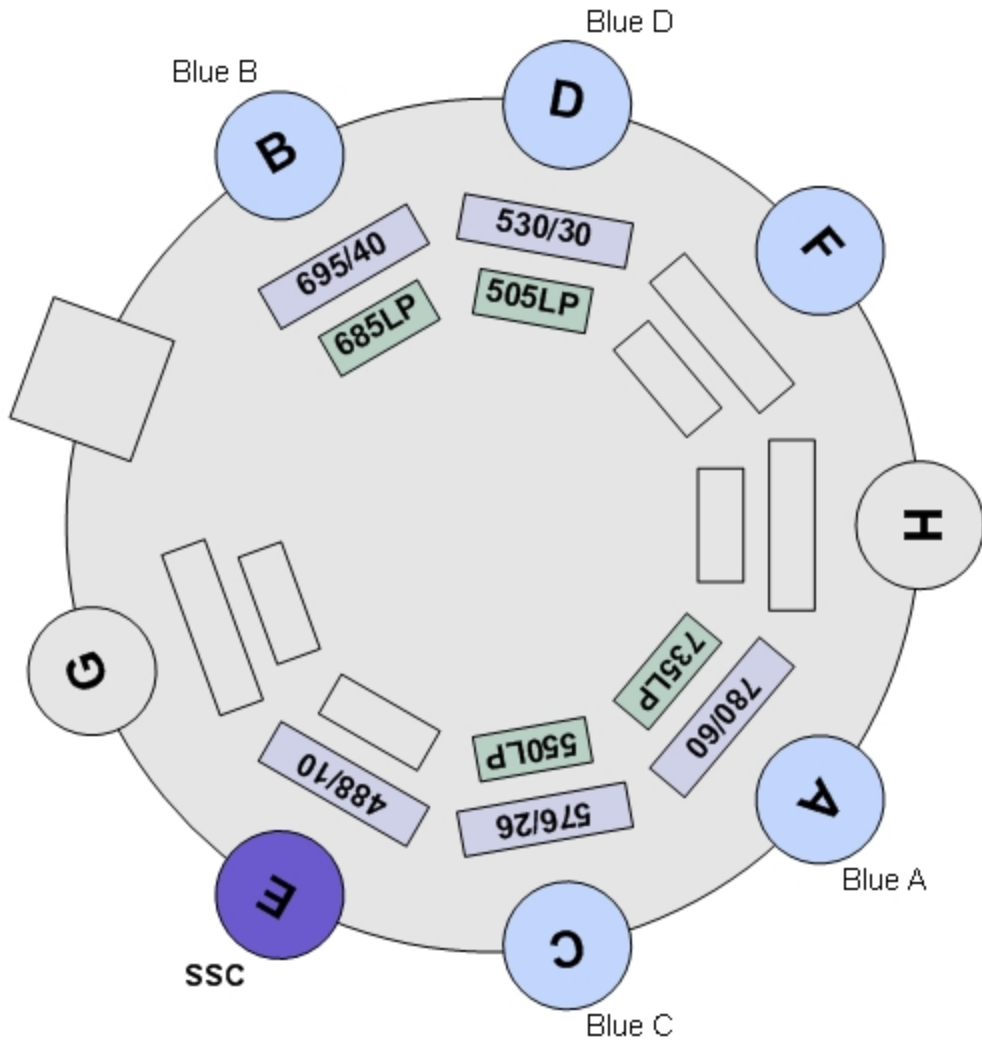


Red Laser  
(640nm)

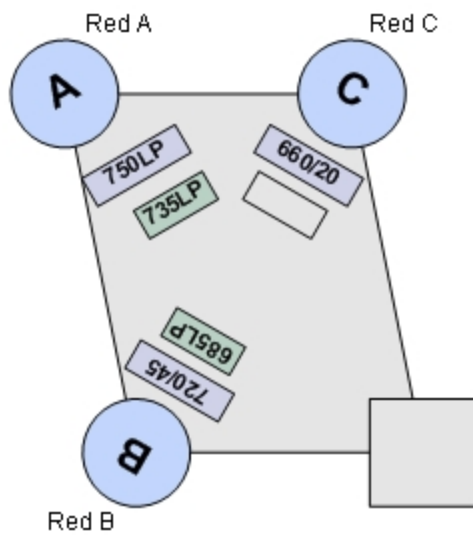

Yellow Green Laser  
(561nm)

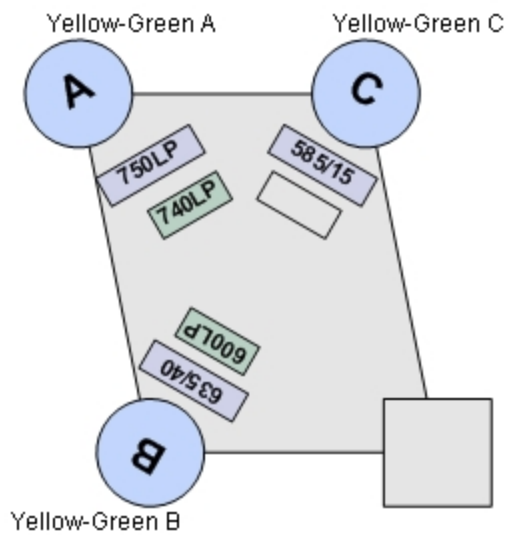

UV Laser  
(355nm)

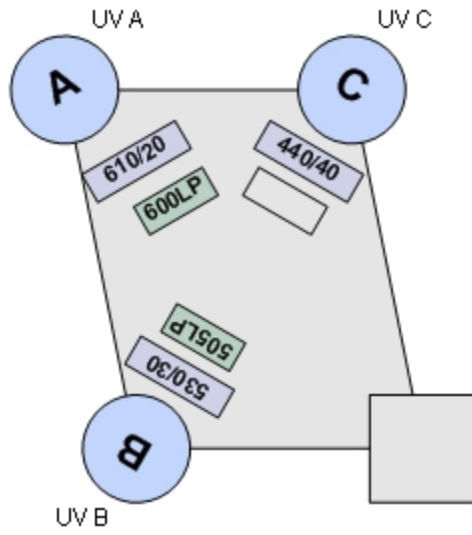

Comments: